

SOLUTION CHANGE

WASHINGTON CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 100284




Date: 05/01/2019

OPERATOR NAME:  
MATTHEW K JACKSON  
Permit #: 40078  
Operator Agency/Dept: WASHINGTON CO. SO  
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:49
INTERNAL STANDARD	VERIFIED	11:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:49
BLANK TEST	0.00	11:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:50
BLANK TEST	0.00	11:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:52
BLANK TEST	0.00	11:53

*MKJ #693*

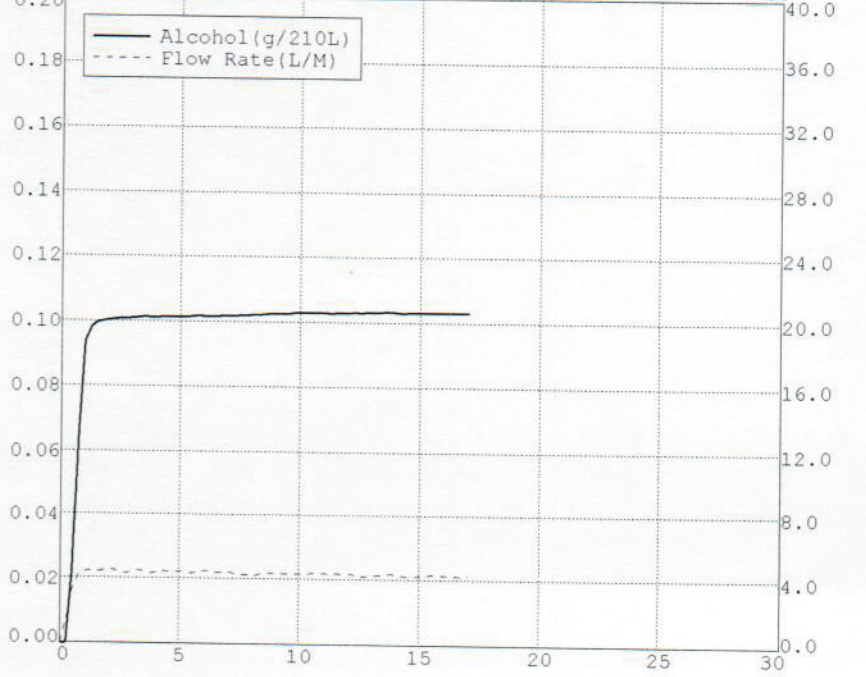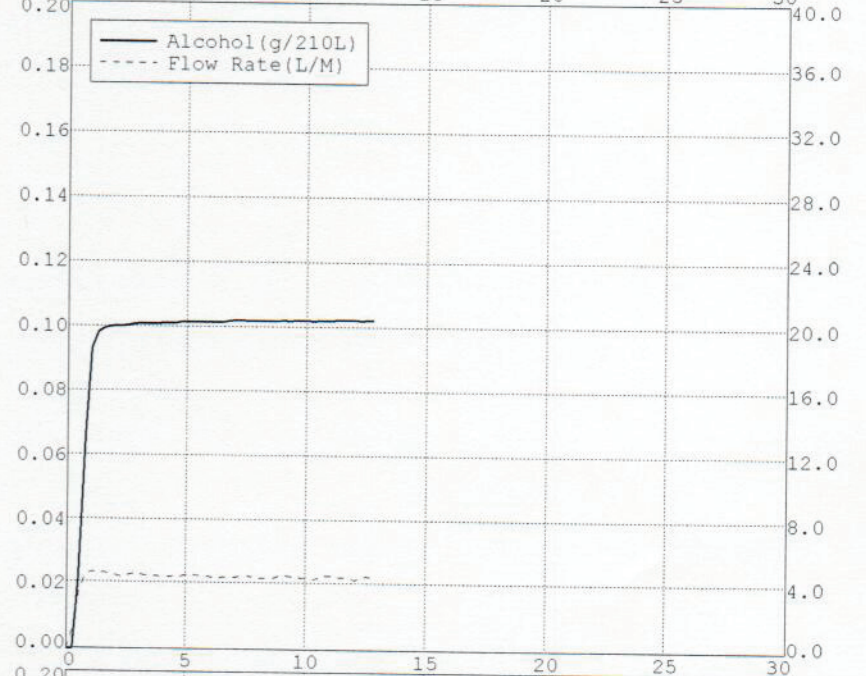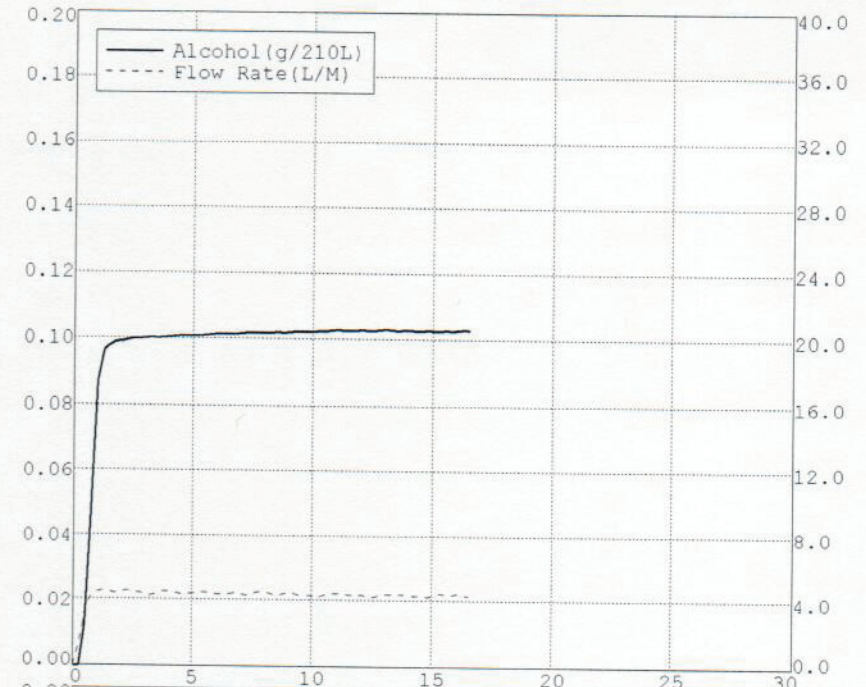

SUPERVISOR TEST

-----  
WASHINGTON CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 100284  
-----

Date: 05/01/2019

OPERATOR NAME:  
MATTHEW K JACKSON  
Permit #: 40078  
Operator Agency/Dept: WASHINGTON CO. SO  
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:15
INTERNAL STANDARD	VERIFIED	01:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:15
BLANK TEST	0.00	01:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:16
BLANK TEST	0.00	01:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:18
BLANK TEST	0.00	01:18

*MRD #693*

