

SUPERVISOR TEST




WASHINGTON CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 100284

Date: 09/23/2019

OPERATOR NAME:
ROBERT J SULLIVAN
Permit #: 34106
Operator Agency/Dept: WASHINGTON CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:06
INTERNAL STANDARD	VERIFIED	03:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:07
BLANK TEST	0.00	03:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:08
BLANK TEST	0.00	03:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:09
BLANK TEST	0.00	03:10

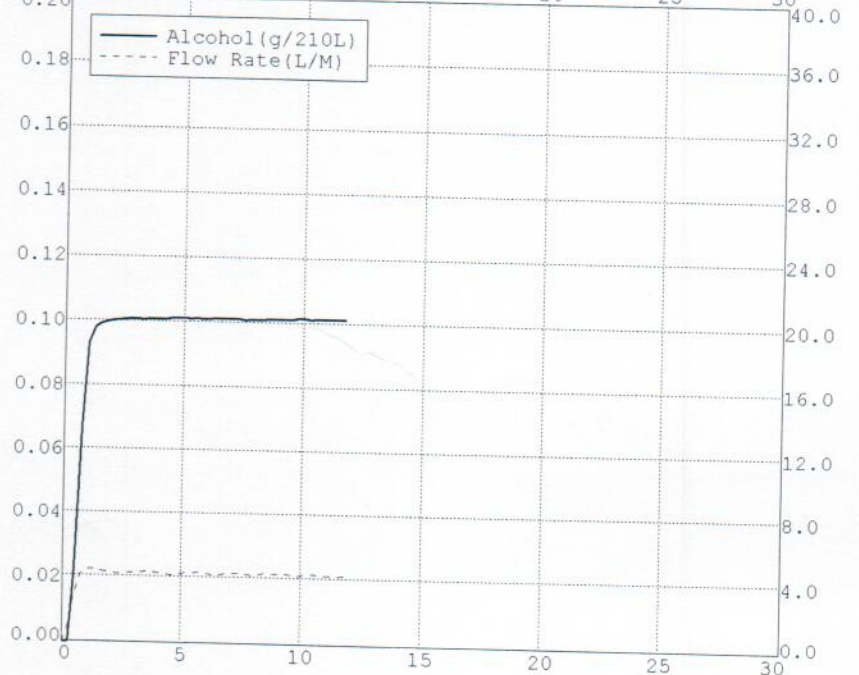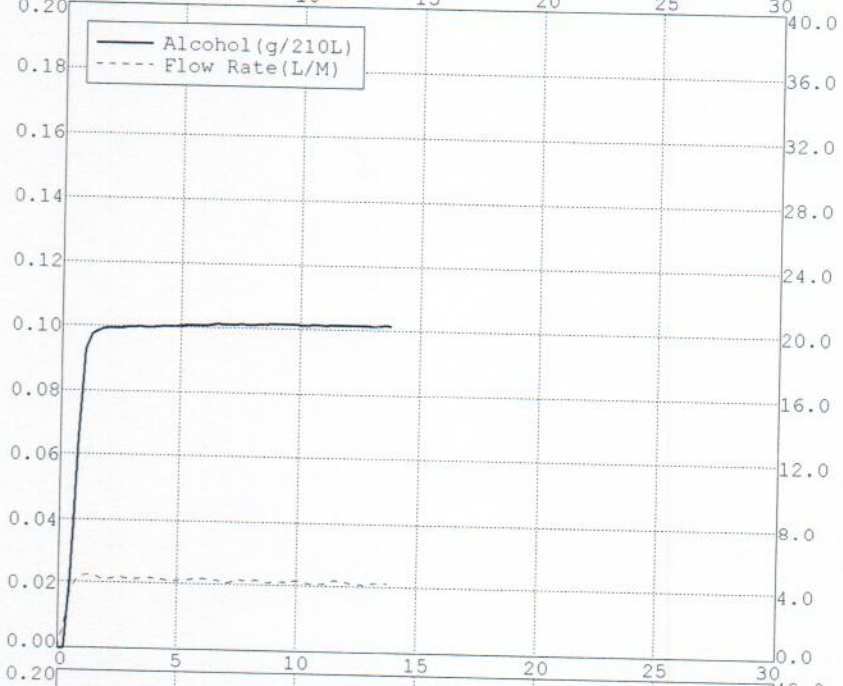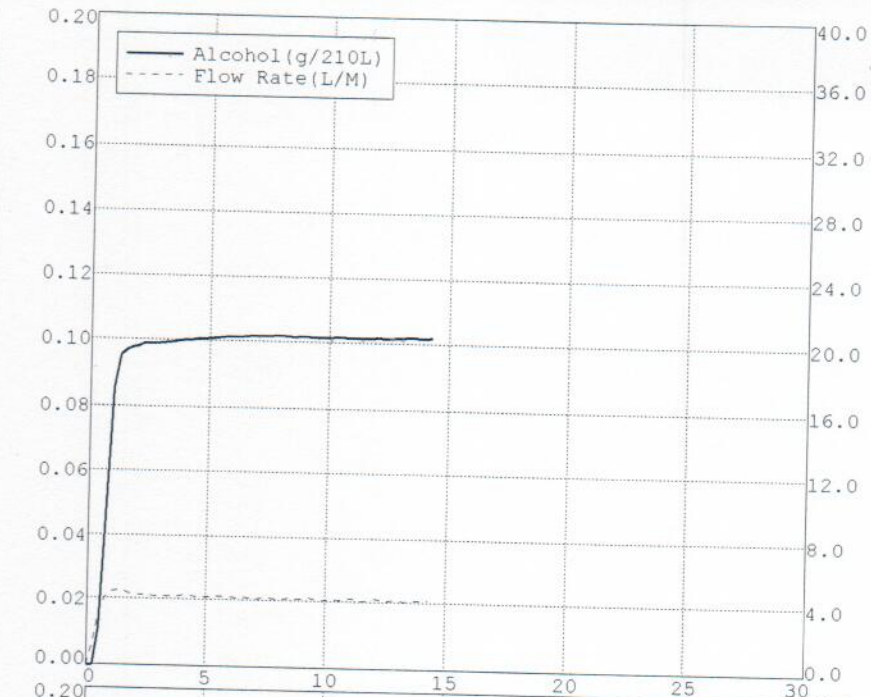

[Handwritten Signature] 688